

© [2008] IEEE. Reprinted, with permission, from [Leijdekkers, P.; Gay, V. A Self-Test to Detect a Heart Attack Using a Mobile Phone and Wearable Sensors. 21st IEEE International Symposium on Computer-Based Medical Systems, 2008. CBMS '08.]. This material is posted here with permission of the IEEE. Such permission of the IEEE does not in any way imply IEEE endorsement of any of the University of Technology, Sydney's products or services. Internal or personal use of this material is permitted. However, permission to reprint/republish this material for advertising or promotional purposes or for creating new collective works for resale or redistribution must be obtained from the IEEE by writing to pubs-permissions@ieee.org. By choosing to view this document, you agree to all provisions of the copyright laws protecting it

A self-test to detect a heart attack using a mobile phone and wearable sensors

Peter Leijdekkers and Valérie Gay

Faculty of IT, University of Technology Sydney
UTS FIT, PO box 123, Broadway 2007 NSW Australia

[Peter.Leijdekkers, Valerie.Gay]@uts.edu.au

Abstract

This paper describes a heart attack self-test application for a mobile phone which allows potential victims of a heart attack to quickly assess whether they are having a heart attack without the intervention of a medical specialist. Heart attacks can occur anytime, anywhere. Using pervasive technology such as a mobile phone and a small wearable ECG sensor it is possible to collect the user's symptoms and to detect the onset of a heart attack by analysing the ECG recordings. If the application assesses that the user is at risk, it will urge the user to call the emergency service immediately. If the user has a cardiac arrest the application will automatically determine the current location of the user and alert the ambulance services and others to the person's location.

1. Introduction

Cardiovascular disease is the leading cause of mortality in the developed world. It refers to various medical conditions that affect the heart and the blood vessels. These conditions include coronary artery disease, myocardial infarction (heart attack), angina, congestive heart failure, hardening of the arteries, stroke and peripheral vascular disease.

Studies in Australia show that more than two thirds of Australians would not call an ambulance if they thought they were having a heart attack [1]. This is backed up by international studies [2] that indicate that many people are hesitant calling the emergency services or go to the emergency room with symptoms of a heart attack. However, for a heart attack it is extremely important to get treatment as quickly as possible since there is a direct relationship between time-to-treatment and the success of reperfusion (restoration of blood flow to the heart). A heart attack comes with warning signs that are not always recognised by the person. People often confuse a heart attack with indigestion or heart burn. A study in Germany [3] showed that sudden cardiac death does not come out of the blue and people often have typical symptoms as long as 2 hours before cardiac death occurs.

A lot of money and research is spent on making people aware of the warning signs (e.g.[4][5]). Getting patients to recognise the warning signs is not an easy task. Several web sites offer a set of questions to assess whether a person has heart attack symptoms but the questions are not integrated in devices that a user carries all the time.

A challenge is to reduce the delay time between the onset of a heart attack and the call to the emergency services ([2][6]) since early detection and prompt treatment is the key to the success of the clinical outcomes. Another challenge is to reduce the amount of false alerts. A pilot conducted by Aerotel and BroomWell Healthcare in the UK showed that 82% of patients did not need to go to hospital following a test and demonstrated the potential to save 46 millions pounds per year by cutting the unnecessary hospital admissions and visits for chest pain symptoms [7].

To deal with these challenges, fast and accurate diagnosis tools should be at hand where the user can be reminded of the warning signs and also perform a on the spot heart attack self test.

Diagnosis tools exist to detect the onset of a heart attack. They use blood test (e.g.[8]), implants (e.g.[9]) or sensors (e.g.[7]). However none of these allow the user to do a self test with non invasive sensors and without the assistance of a health professional. A research project closest to our solution is managed by Aerotel and Broowell healthcare [7] but they use bulkier sensors and the test has to be conducted by a health professional.

The objective of our research is to use non invasive mobile technology to reduce the delay time and the number of false alarms. To achieve this goal we developed a self-test application using a small wearable ECG sensor and a mobile phone. The application is able to detect the onset of a heart attack and urges the user to call the emergency services, or even do it for him or her.

The target group for our application are users that have had a heart attack and are concerned that they will be struck by another one. Their concerns are backed up by the American Heart Association indicating that people who have had a heart attack

have a sudden death rate that is 4 to 6 times that of the general population [10]. We also target users that have a known heart condition (e.g. irregular heart beat, angina). They would not want to wear an ECG heart monitor all the time but would use it when they wish to monitor their condition in case of an episode.

The heart attack self-test application presented in this paper is integrated in the Personal Health Monitor system (PHM) developed at the University of Technology, Sydney [11] and [12]. The Personal Health Monitor system is capable of monitoring the personal health of its user using a mobile phone and various wireless sensors (see Figure 1). The mobile phone analyses, in real-time, data wirelessly received from the sensors, such as an electrocardiogram (ECG), blood pressure measurements or accelerometer data. The mobile phone can send this data, in real time, to heart specialists. If a person is in danger (cardiac arrest, fall) and is unable to call an ambulance, the mobile phone will automatically determine the current location of the person using WiFi, GSM Cell-id or GPS and sends automated voice and text messages to their cardiologist and other emergency numbers programmed into it.

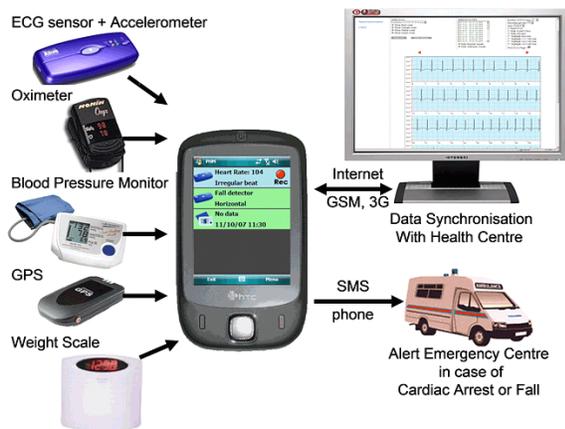


Fig. 1. Personal Health Monitor System.

This paper focuses on the heart attack self-test application and is organised as follows. Section 2 outlines the requirements for the self-test application. Section 3 describes the heart attack self-test application as it is currently implemented on a mobile phone. Section 4 concludes the paper with a discussion.

2. Requirements

Time is a crucial factor in case of a heart attack. If proper medical treatment is performed within 60 minutes of the event, the chances for surviving

improve dramatically and the likelihood of serious damage to heart tissue decreases.

If a person decides to do the self-test, it usually means s/he feels something, and the first priority is to ask whether the person has heart attack related symptoms and analyse the answers. If the symptoms clearly indicate that the person is having a heart attack there is no reason to delay the call to the emergency services. For example, if the user feels pressure in the chest, pain spreading to their left arm, is sweaty and looks extremely pale, the application should immediately urge the person to call the emergency services and not suggest making an additional ECG recording which would delay the process by several minutes.

Automating the call to the emergency service avoids the possibility of dialling the wrong number but more importantly it can also reduce the hesitation many people have not calling the ambulance and hoping that the pain will pass. Talking to the emergency operator could convince the user that urgent treatment is needed.

The accuracy versus time ratio of the diagnosis needs to be optimised. For instance, for the analysis of an ECG, the length of the ECG recording should be minimized but long enough to be able to make an accurate decision.

Time is also a deciding factor how many sensors are used in diagnosing a heart attack. Besides the ECG sensor other sensors (e.g. blood pressure, glucose monitor) will only be used when the emergency level is low.

Simplicity and ease of use is important since most people will be stressed or feeling very uncomfortable, so a quick assessment with minimal interaction is crucial.

The instructions need to be easy to understand. The text displayed on the screen should be large, and the application needs to play (repeatedly) the questions and instructions aloud so that the person does not per se need to read what is displayed on the screen. The interface should take into account that the person might have bad eye sight or be trembling. Answering a question should be as easy as pushing a button on a touch screen.

The sensors have to be simple to operate to lower the threshold for a person to take a measurement. It is important to optimise the accuracy versus ease-of-use ratio for sensors. A 12-lead ECG sensor would be the most accurate one to diagnose a heart attack. But attaching the various cables and placing the electrodes correctly can be difficult without external help from a medical professional. In contrast, a 2-electrodes, 1-lead ECG sensor is easy to attach by a person but offers less

accuracy/information compared to a 12-lead ECG sensor.

A heart attack can happen anytime, anywhere. Therefore the user wants to be able to do the self-test wherever and whenever the symptoms occur. This has an impact on the technology that can be used. The sensors should be small and non intrusive so that people are willing to carry them all the time. A mobile phone is a logical choice for the self-test application to reside on since most people carry one most of the time.

It is important to know some personal details about the user such as age, gender or preferred language to adjust the way it interacts with the person. Medical conditions like prior heart attacks, angina or allergy to certain medicines are important in assessing the probability of a heart attack and to provide the correct feedback to the user (e.g. do not prescribe an aspirin to a person if s/he is allergic to it).

The American Heart Association [13] recommends having easy access to important phone numbers in case of mild to moderate symptoms that do not require the emergency services. The correct phone number to dial varies depending on the time and day. It is therefore important to get contextual information such as date and time. This allows the application to dial automatically the correct number at the day/time the self-test is conducted. Knowing the location is useful if the user has a cardiac arrest to guide the emergency services to the location of the user.

3. The heart attack self-test application

We used these requirements as input for the design of our self-test application. Our objective is therefore to develop a user friendly application able to give quick and accurate feedback to the user anytime, anywhere without intervention of a medical professional.

The user initiates the self-test from the main menu (Figure 2, right) and is requested to answer ‘Yes’ or ‘No’ to several simple questions. The questions are meant to quickly assess what the user is experiencing could be the onset of a heart attack. Based on the answers given and taking into account the personal data and medical history stored in the PHM system, the application decides whether the person is at a high risk of having a heart attack. If at high risk, the application will urge the user to call the emergency services straight away (Figure 3). The emergency number is automatically dialled if the user agrees.

If the answers indicate that the user is at a low risk, or the user declined calling the emergency services, the application will ask the user to carry out two ECG

recordings. The application will analyse these ECG signals for heart attack signs. If they are found, the user will be urged to call the emergency services.



Fig. 2. PHM monitor and the self-test integrated into the PHM application.

If the answers indicate that the user is at a low risk, or the user declined calling the emergency services, the application will ask the user to carry out two ECG recordings. The application will analyse these ECG signals for heart attack signs. If they are found, the user will be urged to call the emergency services.

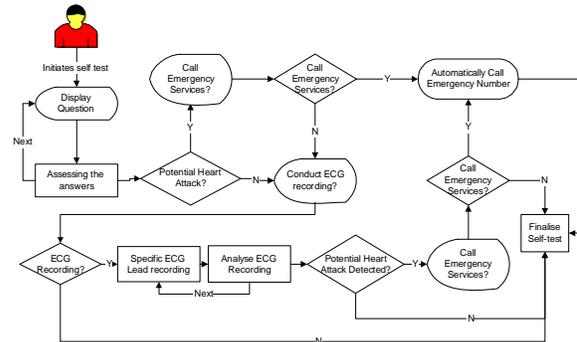


Fig. 3. Flow chart for heart attack self-test

If the self-test application did not detect an abnormality in the ECG signal, the application will finalise the test based on the personal user information available on the PHM system. For example, it advises the user to wear the ECG monitor for that day so that the person is continuously monitored in case of a cardiac arrest.

The following sections describe parts of the process and how they are implemented on the mobile phone.

3.1. Questioning the user

When the person initiates the self-test a series of questions are asked to identify the possible occurrence of a heart attack. The questions (see table 1) are a

compilation of typical heart attack related symptoms as described in [4] and [5]. Symptoms can be different for women and men but we ask enough questions that cover the symptoms for both genders.

Table 1. Questions related to heart attack symptoms.

1.	Do you feel discomfort around your chest? This can be a feeling of tightness, pressure or squeezing in your chest.
2.	Do you feel pain spreading to your shoulders, shoulder-blades, neck or arms?
3.	Are you having indigestion (gas-like pain) or heartburn?
4.	Do you feel nauseous? Did you vomit?
5.	Do you feel dizzy, weak or anxious?
6.	Are you sweaty or short of breath?
7.	Do you look tired, pale?
8.	Do you feel atypical sensations? For example, feelings of overwhelming doom?

Figure 4 shows how the questions are presented to the user on a mobile device. A recorded voice will repeatedly phrase the question so that he person does not need to read it from the screen. If the person is too unwell and not able to handle the phone a family member or any person nearby can assist going through the questions.

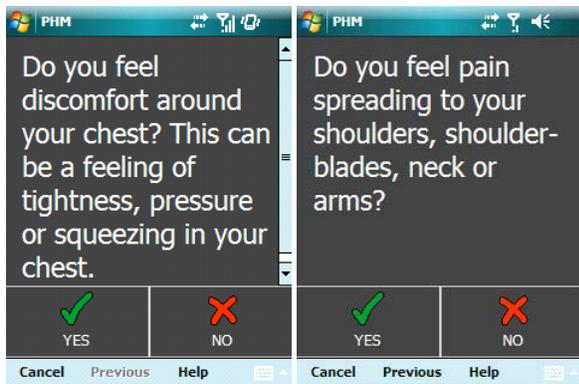


Fig. 4. Screenshot of questions being asked.

The current version of the decision algorithm is basic. If one or more questions are answered positively, the application will urge the person to call the emergency services. Further research is needed to fine-tune the decision algorithm to reduce false alarms but currently we have a “better save than sorry” approach. Further research needs to be conducted to refine the set of questions, adapt them to the user’s condition and take into account extra contextual information (e.g. we can get an indication that the user

was very active before the test using the accelerometer data).

Another example: There are similarities between angina and a heart attack where the location and the severity of the pain can be similar [14]. Angina is usually related to exercise, stress, or after a meal and lasts less than 20 minutes while a heart attack lasts more than 20 minutes and may come and go. Both have symptoms of shortness of breath and dizziness but sweating, nausea, and vomiting are not experimented during an angina. Angina is relieved with rest and/or nitro-glycerine but not in case of a heart attack. Therefore the decision algorithm should be able to distinguish between angina and a heart attack and in case of angina; the advice is to rest, take nitro-glycerine as prescribed and continue monitoring.

3.2. Calling the Emergency Services

The application will automatically dial after 20 seconds. The user is given the option to cancel the call but the idea behind automatic calling is to persuade the user to act. Studies in the UK showed that “*the delay between the time of onset of symptoms and the time at which the patient comes under medical attention is a major determinant of prognosis in acute MI; the largest single component of the delay is that taken by the patient deciding to summon help.*” [15]

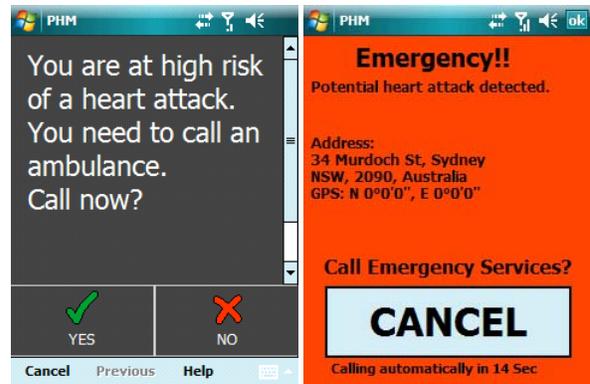


Fig. 5. Automatic call to the emergency services.

Ingafield identified reasons why patients with chest pain delayed seeking hospital medical care and when they do or don’t use an ambulance [16]. One of the observations is that patients see their general practitioner (GP) first which on average resulted in a delay of 30 min. This is confirmed by another study [17] which concludes that most patients who contact non-ambulance services are seen by general practitioners which delayed treatment significantly longer. Based on these studies we decided the call the emergency services first in case of a high risk.

3.3. ECG recording

If the answers suggest no immediate emergency, the application will ask the user to take two ECG recordings where the application will analyse the recordings for signs of a myocardial infarction (MI). During a typical acute myocardial infarction the ECG evolves through three stages [18]:

1. T wave peaking followed by T wave inversion,
2. ST segment elevation,
3. Appearance of new Q waves.

Using the 2-electrodes, 1-lead ECG sensor the application instructs step-by-step where to place the 4 electrodes on the body and how to attach and operate the ECG monitor. We take 2 separate ECG recordings (Figure 6, left and middle) which results in 2 different views on the heart and gives a higher chance to detect MI.

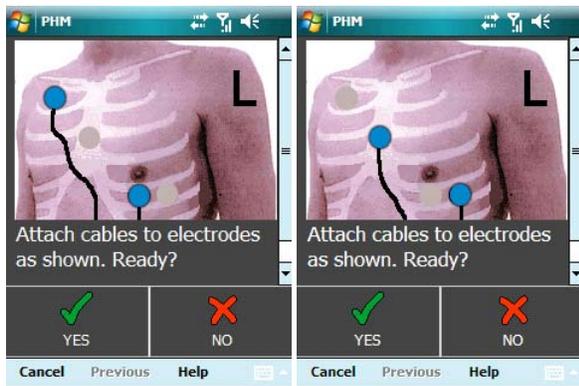


Fig. 6. Obtaining two different ECG recordings

The user will be instructed not to move during the recording to reduce motion artefacts. The application records for 2 minutes and then analyses the ECG recording for changes in the ST segment. Figure 7 shows an example of a normal heart beat (Fig.7, left) and a heartbeat that shows ST elevation (Fig. 7, right) possibly indicating a myocardial infarction. MI can often be seen on an ECG by a flat, down sloping, or depressed ST segments or an ST segment elevation.

We implemented the algorithm developed by P. Langley et al [19] since they achieved the best accuracy for distinguishing ischemic and non-ischemic ST changes in an ambulatory ECG monitor. For the first implementation of our algorithm we focus on ST segment changes since this gives a fairly good indication of an onset of MI. The details and performance of the ST algorithm will be published in a forthcoming paper. When the algorithm detects ischemic events the user will be urged to call the emergency services.

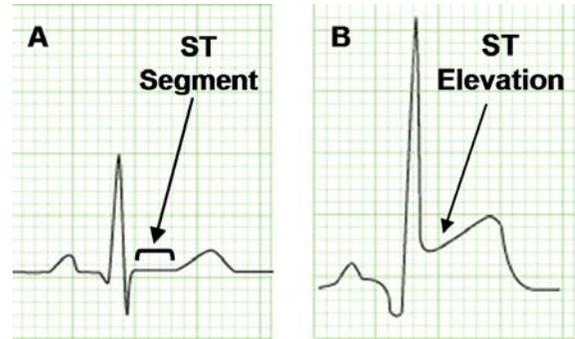


Fig. 7. A normal heart beat and a heartbeat during a myocardial infarction.

3.4. Finalise Self-test

If the emergency services are called, the application will give advice to the victim and bystanders while waiting for the ambulance to arrive. Advice is displayed and played in a recorded message.

The emergency operator might be on the phone providing additional advice which should be followed.

If no heart attack symptoms are found, the application advises the user to wear the ECG monitor for the rest of the day so that the person is continuously monitored by the personal health monitor. The results of the self-test are automatically upload to the health-centre website and can be directly inspected by a health professional. Uploading the ECG recordings to a healthcare centre is important since there are limits to what can be analysed on the mobile phone. The expertise of medical staff is needed to complement the analysis. A health professional can contact the person directly on the mobile phone if irregularities are seen that need immediate treatment.

4. Discussion

The objective of our self-test application is to reduce the delay time between the onset of a heart attack and the call to the emergency services. Two factors contribute to this delay time which are the failure to recognise typical heart attack symptoms and the failure to act [20].

Our self-test solves these issues by using pervasive technology: a mobile phone and a small wearable ECG sensor which can be easily carried by the person. By asking a set of questions, the person will realise what they experience can be a heart attack. The application also analyses two ECG recordings on the mobile phone for heart attack signs to confirm this. Therefore, the application can quickly assess the user's condition and provide appropriate advice without the intervention of a medical professional. It also guides the user and

(potential) bystanders in getting the right help by automating the call.

We record and analyse an ECG in real-time on the mobile phone using a 2 electrode, 1-lead heart monitor developed by Alive technologies [21]. Our algorithm is able to detect heart rhythm abnormalities such as ventricular tachycardia/fibrillation [22] (cardiac arrest) and changes in the ST-segment. We are currently validating whether a 2-electrode heart monitor provides sufficient quality signal for detecting ST segment variations. If this is not the case we can easily switch to a more sophisticated ECG sensor such as the 12-lead ECG sensor developed by Corscience [23]. The downside is that it is a less portable ECG sensor and it will be more difficult to attach the electrodes.

The self-test application is never going to provide 100% accuracy. However, we aim at reducing the false positives (i.e. user has a heart attack and it is not identified) and also bring down the false negatives (i.e. user has not a heart attack but system sees it as a heart attack). We hope to achieve this goal by using a combination of questions and ECG recordings. We are conducting trials with the Personal Health Monitor system at the Royal North Shore Hospital in Sydney and we are investigating the possibility to trialling our self-test application with the same hospital to find out whether it reduces the delay time and therefore improves the outcome for heart attack victims.

5. References

- [1] Australian Heart Foundation, Newpoll research, www.heartfoundation.org.au (2007).
- [2] Schull, M. J.: What are we waiting for? Understanding, measuring and reducing treatment delays for cardiac patients. In: *Emergency Medicine Australasia* 17:3, 191–192 (2005).
- [3] Agrawal, R., Arntz, H.R.: Sudden cardiac death does not always happen without warning. In: *American Heart Association journal report* (2006).
- [4] American Heart Association, www.americanheart.org (2007).
- [5] British Heart foundation, www.bhf.org.uk (2007).
- [6] Moser, D.K., McKinley, S., Dracup, K., Chung, M.L.: Gender differences in reasons patients delay in seeking treatment for acute myocardial infarction symptoms. In: *Patient Education and Counseling* Vol 56 pp 45-54, Elsevier (2005).
- [7] Aerotel website : BroomWell won the HSJ Award 2007 for Improving Care with E-Technology using Aerotel's Wireless Cardiac Monitoring Devices, www.aerotel.com. (2007)
- [8] University of Ulster : Whole-Blood Sensor Research Could Transform Cardiac Testing, *ScienceDaily*. <http://www.sciencedaily.com/releases/2007/10/071020114644.htm> (2007)
- [9] Angel Medical Systems : DETECT Feasibility Study <http://www.angel-med.com/clinical.html>. (2007)
- [10] American Heart Association. *Heart Disease and Stroke Statistics 2005 Update*. Dallas, Texas: American Heart Association (2005).
- [11] Gay, V., Leijdekkers, P.: A Health Monitoring System Using Mobile phones and Wearable Sensors'. In: *Special Issue on 'Smart Sensors in Smart Homes' International Journal of Assistive Robotics and Mechatronics (IJARM)*, ISSN: 1975-0153, pp 29-36, Vol. 8, No. 2, (2007).
- [12] Personal Health Monitor website, www.personalhealthmonitor.net (2007).
- [13] American Heart Association - Cardiac rehabilitation section, Medical Contact List, www.americanheart.org/presenter.jhtml?identifier=304813.
- [14] Angina vs heart attack, Canadian Cardiac Rehabilitation Foundation web site www.cardiacrehabilitation.ca/documents/anginavsheartattack.php.
- [15] Penny W. J.: Patient delay in calling for help: the weakest link in the chain of survival? *Editorial Heart*; 85:121-122, heart.bmj.com/cgi/content/full/85/2/121#B3 (2001).
- [16] Ingarfield, S. L., Jacobs, I.G., Jelinek G.A., Mountain, D.: Patient delay and use of ambulance by patients with chest pain. In: *Emergency Medicine Australasia* 17 (3), 218–223 (2005).
- [17] Hitchcock, T., Rossouw, F., McCoubrie, D., Meek, S.: Observational study of prehospital delays in patients with chest pain. In: *Emerg Med J*; 20: 270-273.(2003).
- [18] Thaler, M.S.: *The Only EKG Book You'll Ever Need*. Paperback, Lippincott Williams & Wilkins; 4 edition, ISBN-10: 0781741769 (2002).
- [19] Langley, P. Bowers, E.J. Wild, J. Drinnan, M.J. Allen, J. Sims, A.J. Brown, N. Murray, A.: An algorithm to distinguish ischaemic and non-ischaemic ST changes in the Holter ECG. In: *Computers in Cardiology*, pp 239- 242, 0276-6547.(2003).
- [20] Finn, J.C., J.H.N. Bett, Shilton, T.R., Cunningham, C., Thompson P. L.: Patient delay in responding to symptoms of possible heart attack: can we reduce time to care? In *Position statement on behalf of the National Heart Foundation of Australia 'Chest Pain Every Minute Counts Working Group'*, *MJA*, Volume 187 Number 5 (2007).
- [21] Alive Technologies website, www.alivetec.com (2007)
- [22] Fokkenrood, S., Leijdekkers, P., Gay, V.: Ventricular Tachycardia/Fibrillation Detection Algorithm for 24/7 Personal Heart Monitoring. In: *ICOST 2007 on Pervasive Computing Perspectives for Quality of Life Enhancement*, pp 110-120, ISBN: 3-540-73034-6. Nara, Japan, (2007).
- [23] Corscience website; 12-channel ECG Device with Bluetooth Functionality, www.corscience.de/12-channel-ecg-device-with-bluetooth.37.en.html, (2007).